



High Sensitivity

SALIVARY 17 β -ESTRADIOL

ENZYME IMMUNOASSAY KIT

For Research Use Only
Not for use in Diagnostic Procedures

Item No. 1-3702, (Single) 96-Well Kit;
1-3702-5, (5-Pack) 480 Wells



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

TABLE OF CONTENTS

Intended Use	3
Introduction	3
Test Principle	4
Safety Precautions	4
General Kit Use Advice	5
Storage	5
pH Indicator	5
Specimen Collection	6
Sample Handling and Preparation	6
Materials Supplied with Single Kit	7
Materials Needed But Not Supplied	8
Reagent Preparation	9
Procedure	10
Quality Control	12
Calculations	12
Typical Results	12
Limitations	13
Salivary 17 β -Estradiol Example Ranges	13
HS Salivary 17 β -Estradiol EIA Kit Performance Characteristics	14
References	18
Seller's Limited Warranty	19



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

Intended Use

The Salimetrics® 17 β -Estradiol Enzyme Immunoassay Kit is a competitive immunoassay specifically designed and validated for the quantitative measurement of salivary Estradiol. It is not intended for diagnostic use. It is intended only for research use in humans and some animals. Salimetrics has not validated this kit for serum or plasma samples.

Warning: The drug fulvestrant (FASLODEX®) has been shown to cross react with antibodies used in Estradiol immunoassays and may cause falsely elevated Estradiol results. Due to the risk of this cross reactivity, the Salimetrics® High Sensitivity Salivary 17 β -Estradiol Enzyme Immunoassay Kit should not be used for individuals being treated with the drug fulvestrant (FASLODEX®). Fulvestrant (FASLODEX®) is used to treat a certain type of estrogen receptor positive breast cancer in postmenopausal women. Falsely elevated Estradiol results could lead to misinterpretation of the menopausal status of these women, resulting in the fulvestrant (FASLODEX®) treatment being incorrectly altered or discontinued.

Please read the complete kit insert before performing this assay. Failure to follow kit procedure and recommendations for saliva collection and sample handling may result in unreliable values.

For further information about this kit, its application, or the procedures in this insert, please contact the technical service team at Salimetrics or your local sales representative.

Introduction

Estradiol (17 β -Estradiol, E2, 1,3,5(10)-estratriene-3, 17 β -diol), a steroid hormone, is produced primarily by the ovarian follicles from testosterone (1,2). Estradiol is the most active naturally secreted estrogen (1). In men, Estradiol originates in the testes and from extraglandular conversion of androgens (1).

Circulating Estradiol levels are relatively high at birth in both males and females, but decrease postnatally (2). In prepubertal children and men, levels are non-cyclic and low. During puberty, there are gradual increases in Estradiol levels in both males and females. Interactions between luteinizing hormone (LH) and follicle-stimulating hormone (FSH) cause the release of Estradiol from the ovaries in premenopausal women. Estradiol secretion is low in postmenopausal women.

Research concerning Estradiol has focused predominantly on reproductive issues such as conception, ovulation, infertility, and menopause (3,4). Yet, Estradiol affects a diversity of biological processes involved with reproductive capacity, (5) establishment and maintenance of pregnancy, (6) parenting, (7) coronary artery disease, (8) immunocompetence, (9) cancer susceptibility, (10) and neuroprotection (11). Estradiol is also believed to affect individual differences in cognitive and socioemotional processes as well as psychopathology (12,13).



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

Estrogens have been measured by many immunoassay methods. Studies suggest that Estradiol can be accurately measured in saliva (3,4,14,15).

Test Principle

This is a competitive immunoassay kit. Estradiol in standards and samples compete with Estradiol conjugated to horseradish peroxidase for the antibody binding sites on a microtitre plate. After incubation, unbound components are washed away. Bound Estradiol Enzyme Conjugate is measured by the reaction of the horseradish peroxidase enzyme to the substrate tetramethylbenzidine (TMB). This reaction produces a blue color. A yellow color is formed after stopping the reaction with an acidic solution. The optical density is read on a standard plate reader at 450 nm. The amount of Estradiol Enzyme Conjugate detected is inversely proportional to the amount of Estradiol present in the sample (16).

Safety Precautions

Read Safety Data Sheets before handling reagents.

Hazardous Ingredients

Liquid Stop Solution is caustic; use with care. We recommend the procedures listed below for all kit reagents.

Handling

Follow good laboratory practices when handling kit reagents. Laboratory coats, gloves, and safety goggles are recommended. Wipe up spills using appropriate absorbent materials while wearing protective clothing. Follow local regulations for disposal.

Emergency Exposure Measures

In case of contact, immediately wash skin or flush eyes with water for 15 minutes. Remove contaminated clothing. If inhaled, remove individual to fresh air. If individual experiences difficulty breathing call a physician.

The above information is believed to be accurate but is not all-inclusive. This information should be used only as a guide. Salimetrics will not be liable for accidents or damage resulting from misuse of product.

Safety Data Sheets are available by contacting Salimetrics at support@salimetrics.com (See www.salimetrics.com for alternative contact options).



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

General Kit Use Advice

- This kit uses break-apart microtitre strips. You may run less than a full plate. Unused wells must be stored at 2-8°C in the foil pouch with desiccant and used in the frame provided.
- Avoid microbial contamination of opened reagents. Salimetrics recommends using opened reagents within one month. Store all reagents at 2-8°C.
- The quantity of reagent provided with a single kit is sufficient for three partial runs. The volumes of wash buffer and enzyme conjugate prepared for assays using less than a full plate should be scaled down accordingly, keeping the same dilution ratio.
- Do not mix components from different lots of kits.
- To ensure highest quality assay results, pipetting of samples and reagents must be done as quickly as possible (without interruption) across the plate. Ideally, the process should be completed within 20 minutes or less.
- When using a multichannel pipette to add reagents, always follow the same sequence when adding all reagents so that the incubation time is the same for all wells.
- When running multiple plates, or multiple sets of strips, a standard curve must be run with each individual plate and/or set of strips.
- The temperature of the laboratory may affect assays. Salimetrics' kits have been validated at 68-74°F (20-23.3°C). Higher or lower temperatures may affect OD values.
- Routine calibration of pipettes and other equipment is critical for the best possible assay performance.
- When mixing plates during assay procedures, avoid speeds that spill the contents of the wells.

Storage

All unopened components of this kit are stable at 2-8°C until the kit's expiration date.

pH Indicator

Estradiol values from samples with a pH \leq 5.0 or \geq 9.0 may be inaccurate. A pH indicator in the HS Estradiol Assay Diluent alerts the user to samples with high or low pH values. Upon addition of the HS Estradiol Assay Diluent, acidic samples will turn yellow and alkaline samples will turn purple. Dark yellow or purple wells indicate that a pH value for that sample should be obtained using pH strips. Samples with a pH \leq 5.0 or \geq 9.0 should be recollected.



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

Specimen Collection

Avoid sample collection within 60 minutes after eating a major meal or within 12 hours after consuming alcohol. Acidic or high sugar foods can compromise assay performance by lowering sample pH and influencing bacterial growth. To minimize these factors, rinse mouth thoroughly with water 10 minutes before sample is collected.

Collect whole saliva by unstimulated passive drool. Donors may tilt the head forward, allowing the saliva to pool on the floor of the mouth, then pass the saliva through the SalivaBio Collection Aid (SCA) into a polypropylene vial. Collection protocols/methods are available online at www.salimetrics.com or upon request.

Samples visibly contaminated with blood should be recollected. Samples may be screened for possible blood contamination (17,18) using our Blood Contamination EIA Kit (Item Nos. 1-1302/1-1302-5). Do not use dipsticks, which result in false positive values due to salivary enzymes.

Record the time and date of specimen collection.

Sample Handling and Preparation

After collection, it is important to keep samples cold in order to avoid bacterial growth in the specimen. Refrigerate sample within 30 minutes, and freeze at or below -20°C within 4 hours of collection. (Samples may be stored at -20°C for up to 6 months.) For long term storage, refer to the Salimetrics Collection and Handling Advice Booklet.

Do not add sodium azide to saliva samples as a preservative, as it may cause interference in the immunoassay.

On day of assay, thaw the saliva samples completely, vortex, and centrifuge at 1500 x g for 15 minutes. Freezing saliva samples will precipitate mucins. Centrifuging removes mucins and other particulate matter which may interfere with antibody binding and affect results. Samples should be at room temperature before adding to assay plate. Pipette clear sample into appropriate wells. Re-freeze saliva samples as soon as possible after adding to the assay plate. Re-centrifuge saliva samples each time that they are thawed. Avoid multiple freeze-thaw cycles.



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

Materials Supplied with Single Kit

	Item	Quantity/Size
1	Microtitre Plate Coated with rabbit anti-Estradiol antibodies.	1/96 well
2	HS Estradiol Standard 32 pg/mL, in a saliva-like matrix. Serially dilute before use according to Reagent Preparation. Contains: Estradiol, buffer, preservative.	1 vial / 1.6 mL
3	HS Estradiol Controls High, Low, in a saliva-like matrix. Ready to use. Contain: Estradiol, buffer, preservative.	2 vials / 1 mL each
4	Estradiol Enzyme Conjugate Concentrate. Dilute before use with HS Estradiol Assay Diluent. (See step 5 of Procedure.) Contains: Estradiol conjugated to HRP, preservative.	1 vial / 50 µL
5	HS Estradiol Assay Diluent Contains: phosphate buffer, pH indicator, preservative.	1 bottle / 60 mL
6	Wash Buffer Concentrate (10X) Dilute before use according to Reagent Preparation. Contains: phosphate buffer, detergent, preservative.	1 bottle / 100 mL
7	TMB Substrate Solution Non-toxic, ready to use.	1 bottle / 25 mL
8	Stop Solution	1 bottle / 12.5 mL
9	Non-Specific Binding (NSB) Wells Do not contain anti-Estradiol antibody. Break off and insert as blanks (optional) where needed.	1 strip
10	Adhesive Plate Covers	2



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com


Materials Needed But Not Supplied

- Precision pipette to deliver 15 μL , 100 μL , and 300 μL
- Precision multichannel pipette to deliver 50 μL , 100 μL , and 200 μL
- Vortex
- Plate rotator with 0.08-0.17 inch orbit capable of 500 rpm
- Plate reader with 450 nm and 620 to 630 nm reference filters
- Computer software for data reduction
- Deionized water
- Reagent reservoirs
- One disposable polypropylene tube to hold at least 12 mL
- Five small disposable polypropylene tubes for dilution of standard
- Pipette tips
- Serological pipette to deliver up to 12 mL
- Centrifuge capable of 1500 x g



Reagent Preparation

- Bring all reagents to room temperature and mix before use. A minimum of 1.5 hours is recommended for the 12 mL of HS Estradiol Assay Diluent used in Step 5 (conjugate dilution) to come to room temperature.
- Bring Microtitre Plate to room temperature before use. ***It is important to keep the foil pouch with the plate strips closed until warmed to room temperature, as humidity may have an effect on the coated wells.***
- Prepare 1X wash buffer by diluting Wash Buffer Concentrate (10X) 10-fold with room-temperature deionized water (100 mL of Wash Buffer Concentrate (10X) to 900 mL of deionized water). ***Dilute only enough for current day's use and discard any leftover reagent.*** (If precipitate has formed in the concentrated wash buffer, it may be heated to 40°C for 15 minutes. Cool to room temperature before use in assay.)
- Prepare serial dilutions of the HS Estradiol Standard as follows:
 - Label five polypropylene microcentrifuge tubes or other small tubes 2 through 6.
 - Pipette 300 μ L of HS Estradiol Assay Diluent into tubes 2 through 6.
 - Serially dilute the standard 2X by adding 300 μ L of the 32 pg/mL standard (tube 1) to tube 2. Mix well.
 - After changing pipette tips, remove 300 μ L from tube 2 to tube 3. Mix well.
 - Continue for tubes 4, 5, and 6.
 - The final concentrations of standards for tubes 1 through 6 are, respectively, 32 pg/mL, 16 pg/mL, 8 pg/mL, 4 pg/mL, 2 pg/mL, and 1 pg/mL. Standard concentrations in pmol/L are 117, 58.5, 29, 14.6, 7.3, and 3.65 respectively.

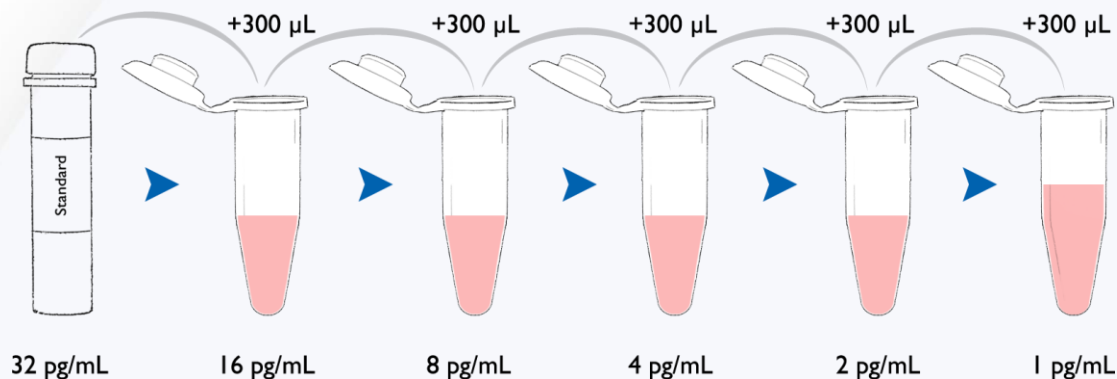

Procedure

Step 1: Read and prepare reagents according to the Reagent Preparation section before beginning assay. Determine your plate layout. Here is a suggested layout. (Standards, controls, and saliva samples should be assayed in duplicate.)

	1	2	3	4	5	6	7	8	9	10	11	12
A	32 Std	32 Std	Ctrl-H	Ctrl-H								
B	16 Std	16 Std	Ctrl-L	Ctrl-L								
C	8 Std	8 Std	SMP-1	SMP-1								
D	4 Std	4 Std	SMP-2	SMP-2								
E	2 Std	2 Std	SMP-3	SMP-3								
F	1 Std	1 Std	SMP-4	SMP-4								
G	Zero	Zero	SMP-5	SMP-5								
H	NSB*	NSB*	SMP-6	SMP-6								

*NSB = Non-specific binding wells. These may serve as blanks. Use is optional.

Step 2: Keep the desired number of strips in the strip holder and place the remaining strips back in the foil pouch. If you choose to place non-specific binding wells in H-1, 2, remove strips 1 and 2 from the strip holder and break off the bottom wells. Place the strips back into the strip holder leaving H-1, 2 blank. Break off 2 NSB wells from the strip of NSB wells included in the foil pouch. Place in H-1, 2. Alternatively, NSBs may be placed wherever you choose on the plate. Reseal the foil pouch with unused wells and desiccant. Store at 2-8°C.

Cautions: *1. Extra NSB wells should not be used for determination of standards, controls, or unknowns.*
2. Do not insert wells from one plate into a different plate.

Step 3: Pipette 12 mL of HS Estradiol Assay Diluent into the disposable tube. (Scale down proportionally if using less than the entire plate.) Set aside for Step 5.

Step 4:

- Pipette 100 µL of standards, controls, and saliva samples into appropriate wells.
- Pipette 100 µL of HS Estradiol Assay Diluent into 2 wells to serve as the zero.
- Pipette 100 µL of HS Estradiol Assay Diluent into each NSB well.



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

Step 5: Dilute the Enzyme Conjugate 1:800 by adding 15 μL of the conjugate to the 12 mL tube of HS Estradiol Assay Diluent. (Scale down proportionally if not using the entire plate.) Conjugate tube may be centrifuged for a few minutes to bring the liquid down to the tube bottom. Immediately mix the diluted conjugate solution and add 100 μL to each well using a multichannel pipette.

Step 6: Place adhesive cover provided over plate. Mix plate on a plate rotator for 5 minutes at 500 rpm and incubate at room temperature for a total of 2 hours.

Step 7: Wash the plate 4 times with 1X wash buffer. A plate washer is recommended. However, washing may be done by gently squirting wash buffer into each well with a squirt bottle, or by pipetting 300 μL of wash buffer into each well and then discarding the liquid over a sink. After each wash, the plate should be thoroughly blotted on paper towels before turning upright. If using a plate washer, blotting is still recommended after the last wash.

Step 8: Add 200 μL of TMB Substrate Solution to each well with a multichannel pipette.

Step 9: Mix on a plate rotator for 5 minutes at 500 rpm and incubate the plate in the dark (covered) at room temperature for an additional 25 minutes.

Step 10: Add 50 μL of Stop Solution with a multichannel pipette.

Step 11:

- Mix on a plate rotator for 3 minutes at 500 rpm. If green color remains, continue mixing until green color turns to yellow. Be sure all wells have turned yellow.

Caution: Spillage may occur if mixing speed exceeds 600 rpm.

- Wipe off bottom of plate with a water-moistened, lint-free cloth and wipe dry.
- Read in a plate reader at 450 nm. Read plate within 10 minutes of adding Stop Solution. (For best results, a secondary filter correction at 620 to 630 nm is recommended.)



Quality Control

The Salimetrics' High and Low Estradiol Controls should be run with each assay. The control ranges established at Salimetrics are to be used as a guide. Each laboratory should establish its own range. Variations between laboratories may be caused by differences in techniques and instrumentation.

Calculations

1. Compute the average optical density (OD) for all duplicate wells.
2. Subtract the average OD for the NSB wells (if used) from the OD of the zero, standards, controls, and saliva samples.
3. Calculate the percent bound (B/Bo) for each standard, control, and saliva sample by dividing the OD of each well (B) by the average OD for the zero (Bo). (The zero is not a point on the standard curve.)
4. Determine the concentrations of the controls and saliva samples by interpolation using data reduction software. We recommend using a 4-parameter non-linear regression curve fit.
5. Samples with Estradiol values greater than 32 pg/mL should be diluted with HS Estradiol Assay Diluent and rerun for accurate results. If a dilution of the sample is used, multiply the assay results by the dilution factor.

A new Standard Curve must be run with each full or partial plate.

Typical Results


The results shown below are for illustration only and should not be used to calculate results from another assay.

Well	Standard	Average OD	B	B/Bo	Estradiol (pg/mL)
A1,A2	S1	0.183	0.174	0.185	32
B1,B2	S2	0.290	0.280	0.299	16
C1,C2	S3	0.438	0.429	0.457	8
D1,D2	S4	0.619	0.609	0.650	4
E1,E2	S5	0.773	0.764	0.814	2
F1,F2	S6	0.837	0.828	0.883	1
G1,G2	Bo	0.947	0.937	NA	NA
H1,H2	NSB	0.009	NA	NA	NA



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

Example: HS 17β-Estradiol 4-Parameter Curve Fit

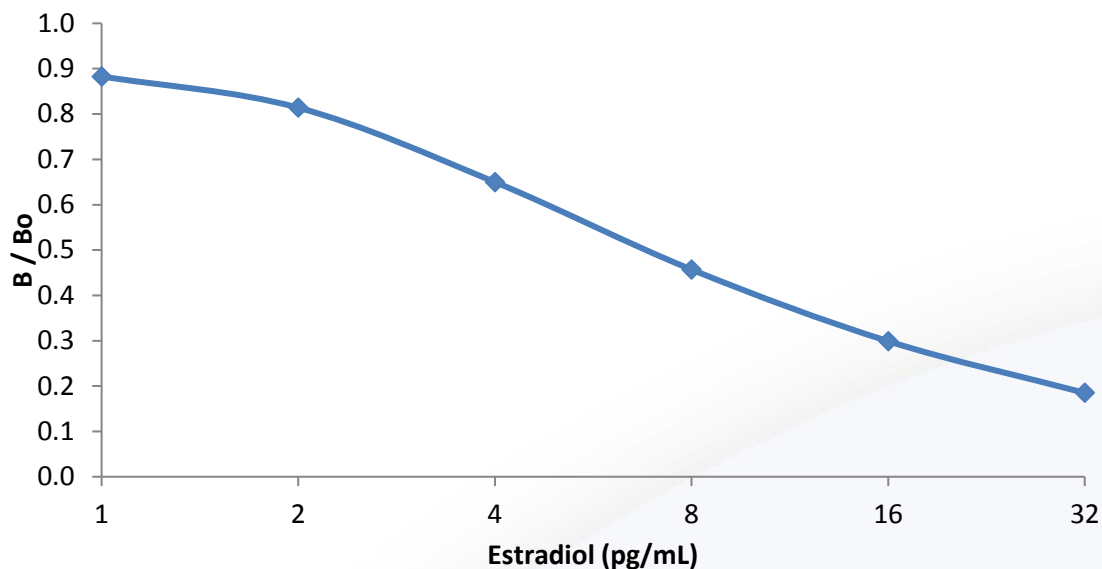

Limitations

- Samples with Estradiol values greater than 32 pg/mL should be diluted with HS Estradiol Assay Diluent and rerun for accurate results. To obtain the final Estradiol concentration, multiply the concentration of the diluted sample by the dilution factor.
- A pH value should be obtained on samples that appear yellow or purple after the diluted conjugate solution is added and the plate is mixed (Step 6). Samples with pH values ≤ 5.0 or ≥ 9.0 should be recollected.
- See "Specimen Collection" recommendations to ensure proper collection of saliva specimens and to avoid interfering substances.
- Samples collected with sodium azide are unsuitable for this assay.
- Any quantitative results indicating abnormal Estradiol levels should be followed by additional testing and evaluation.

Salivary Estradiol Example Ranges*


Pre-menopausal Adult Women	N	Mean (pg/mL)	Standard Deviation (pg/mL)
Follicular	20	1.35	0.80
Mid-Cycle	20	2.97	1.58
Luteal	20	2.56	0.84

*To be used as a guide only. Each laboratory should establish its own range.



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

Example of the Variation of Estradiol Levels during the Menstrual Cycle of One Woman

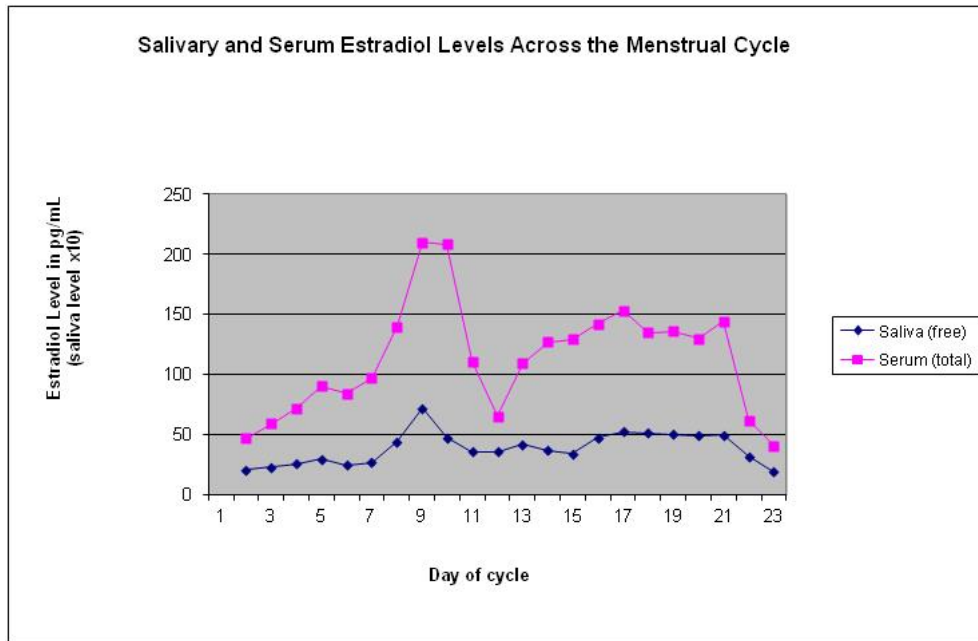

HS Salivary 17 β -Estradiol EIA Kit Performance Characteristics

Precision

The intra-assay precision was determined from the mean of 14 replicates each.

Saliva Sample	N	Mean (pg/mL)	Standard Deviation (pg/mL)	Coefficient of Variation (%)
High	14	20.26	1.42	7.0
Mid	14	7.24	0.45	6.3
Low	14	3.81	0.31	8.1



101 Innovation Boulevard • Suite 302 • State College, PA 16803
 1.800.790.2258 • support@salimetrics.com • salimetrics.com

The inter-assay precision was determined from the mean of average duplicates for 10 separate runs.

Saliva Sample	N	Mean (pg/mL)	Standard Deviation (pg/mL)	Coefficient of Variation (%)
H	10	24.62	1.47	6.0
L	10	4.76	0.42	8.9

Recovery

Five saliva samples containing different levels of endogenous Estradiol were spiked with known quantities of Estradiol and assayed.

Saliva Sample	Endogenous (pg/mL)	Added (pg/mL)	Expected (pg/mL)	Observed (pg/mL)	Recovery (%)
1	2.92	20.48	23.40	23.84	101.9
2	4.68	13.65	18.33	17.91	97.7
3	3.80	3.20	7.00	6.78	96.9
4	5.41	20.48	25.89	28.2	108.9
5	3.69	3.20	6.89	8.26	120.0

Sensitivity

The lower limit of sensitivity was determined by interpolating the mean optical density minus 2 SDs of 10 sets of duplicates at the 0 pg/mL level. The minimal concentration of Estradiol that can be distinguished from 0 is 0.1 pg/mL.

Correlation with Serum

The correlation between serum and saliva Estradiol in females was determined by assaying 11 matched samples. Samples were screened for pH and blood contamination. The magnitude of the serum-saliva correlation, $r(9) = 0.80$, $p = <0.001$, is consistent with the literature (4,15,19).



Sample Dilution Recovery

Four samples were serially diluted with HS Estradiol Assay Diluent and assayed.

Saliva Sample	Dilution Factor	Expected (pg/mL)	Observed (pg/mL)	Recovery (%)
1			28.98	
	1:2	14.49	13.57	93.7
	1:4	7.25	7.24	99.9
	1:8	3.62	3.73	103.0
2			23.84	
	1:2	11.92	12.03	100.9
	1:4	5.96	5.56	93.3
	1:8	2.98	3.60	120.8
3			6.78	
	1:2	3.39	3.07	90.6
	1:4	1.70	1.70	100.0
4			8.54	
	1:2	4.27	4.55	106.6
	1:4	2.14	1.93	90.2



Antibody Specificity

Compound	Spiked Concentration (ng/mL)	% Cross-reactivity in HS 17 β -Salivary Estradiol EIA
Estriol	10	0.234
Estrone	1	1.276
Progesterone	100	ND
17 α -Hydroxyprogesterone	1000	ND
Testosterone	1000	ND
Cortisol	1000	ND
DHEA	1000	ND
Androstenedione	1000	ND
Aldosterone	1000	ND
Cortisone	1000	ND
11-Deoxycortisol	1000	ND
21-Deoxycortisol	1000	ND
Dexamethasone	1000	ND
Triamcinolone	1000	ND
Corticosterone	1000	ND
Prednisolone	1000	ND
Prednisone	100	0.016
Transferrin	1000	ND
Ethinodiol diacetate	1000	ND
Ethinylestradiol	10	0.189

ND = None detected (<0.004)



101 Innovation Boulevard • Suite 302 • State College, PA 16803
 1.800.790.2258 • support@salimetrics.com • salimetrics.com

References

1. Abraham, G.E. (1975). The applications of steroid radioimmunoassay to gynecologic endocrinology. In: M.L. Taymor and T.H. Green (Eds.). *Progress in Gynecology* (Vol. 1), pp. 111-44. New York: Grune and Stratton.
2. Faiman, C., Winter, S. D., & Reyes, F.I. (1976). Patterns of gonadotropins and gonadal steroids throughout life. *Clin Obstet Gynecol*, 3(3), 467-83.
3. Lipson, S.F. & Ellison, P.T. (1996). Comparison of salivary steroid profiles in naturally occurring conception and non-conception cycles. *Hum Reprod*, 11(10), 2090-96.
4. Choe, J.K., Khan-Dawood, F.S., & Dawood, M.Y. (1983). Progesterone and estradiol in saliva and plasma during the menstrual cycle. *Am J Obstet Gynecol*, 147(5), 557-62.
5. Scheffer, G.J., Broekmans, F.J., Looman, C.W., Blankenstein, M., Fauser, B.C., de Jong, F.H., & te Velde, E.R. (2003). The number of antral follicles in normal women with proven fertility is the best reflection of reproductive age. *Hum Reprod*, 18(4), 700-6.
6. Bazer, F.W., Wu, G., Spencer, T.E., Johnson, G.A., Burghardt, R.C., & Bayless, K. (2009). Novel pathways for implantation and establishment and maintenance of pregnancy in mammals. *Mol Hum Reprod*, 16(3), 135-52.
7. Maestriperi, D. (1999). The biology of human parenting: Insights from nonhuman primates. *Neurosci Biobehav Rev*, 23(3), 411-22.
8. Perez-Lopez, F.R., Larrad-Mur, L., Kallen, A., Chedraui, P., & Taylor, H.S. (2010). Gender differences in cardiovascular disease: Hormonal and biochemical influences. *Reprod Sci*, 17(6), 511-31.
9. Gameiro, C.M., Romão, F., & Castelo-Branco, C. (2010). Menopause and aging: Changes in the immune system –A review. *Maturitas*, 67(4), 316-20.
10. Tsuchiya, U., Nakajima, M., & Yokoi, T. (2005). Cytochrome P450- mediated metabolism of estrogens and its regulation in human. *Cancer Lett*, 227(2), 115-24.
11. McEwen, B.S. (1999). The molecular and neuroanatomical basis for estrogen effects in the central nervous system. *J Clin Endocrinol Metab*, 84(6), 1790-97.
12. Uvnas-Moberg, K., Widstrom, A., Nissen, E., & Bjorvell, H. (1990). Personality traits in women 4 days postpartum and their correlation with plasma levels of oxytocin and prolactin. *Psychosom Obstet Gynaecol*, 11, 261-73.
13. Seeman, M.V. (1997). Psychopathology in women and men: Focus on female hormones. *Am J Psychiatry*, 154(12), 1641-47.
14. Shirtcliff, E. A., Granger, D.A., Schwartz, E., & Curran, M.J. (2001). Use of salivary biomarkers in biobehavioral research: Cotton-based sample collection methods can interfere with salivary immunoassay results. *Psychoneuroendocrinology*, 26(2), 165-73.
15. Shirtcliff, E.A., Granger, D.A., Schwartz, E.B., Curran, M.J., Booth, A., & Overman, W.H. (2000). Assessing estradiol in biobehavioral studies using saliva and blood spots: Simple radioimmunoassay protocols, reliability, and comparative validity. *Horm Behav*, 38(2), 137-47.
16. Chard, T. (1990). *An introduction to radioimmunoassay and related techniques* (4th ed.). Amsterdam: Elsevier.
17. Kivlighan, K.T., Granger, D.A., Schwartz, E.B., Nelson, V., Curran, M., & Shirtcliff, E.A. (2004). Quantifying blood leakage into the oral mucosa and its effects on the measurement of cortisol, dehydroepiandrosterone, and testosterone in saliva. *Horm Behav*, 46(1), 39-46.



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com

18. Schwartz, E. & Granger, D.A. (2004). Transferrin enzyme immunoassay for quantitative monitoring of blood contamination in saliva. *Clin Chem*, 50(3), 654-56.
19. Ellison, P.T. (1999). Salivary estradiol—A viable alternative? *Fertil Steril*, 72(5), 951-52.

Seller's Limited Warranty

"Seller warrants that all goods sold hereunder will be free from defects in material and workmanship. Upon prompt notice by Buyer of any claimed defect, which notice must be sent within thirty (30) days from date such defect is first discovered and within three months from the date of shipment, Seller shall, at its option, either repair or replace the product that is proved to Seller's satisfaction to be defective. All claims should be submitted in written form. This warranty does not cover any damage due to accident, misuse, negligence, or abnormal use. Liability, in all cases, will be limited to the purchased cost of the kit.

It is expressly agreed that this limited warranty shall be in lieu of all warranties of fitness and in lieu of the warranty of merchantability. Seller shall not be liable for any incidental or consequential damages that arise out of the installation, use or operation of Seller's product or out of the breach of any express or implied warranties."

Salimetrics, LLC
5962 La Place Court, Suite 275
Carlsbad, CA 92008, USA
(T) 760.448.5397
(F) 814.234.1608
800-790-2258 (USA & Canada only)
www.salimetrics.com
support@salimetrics.com

Salimetrics, LLC
101 Innovation Blvd., Suite 302
State College, PA 16803, USA
(T) 814.234.2617
(F) 814.234.1608
800-790-2258 (USA & Canada only)
www.salimetrics.com
support@salimetrics.com

Updated: April 19, 2019



101 Innovation Boulevard • Suite 302 • State College, PA 16803
1.800.790.2258 • support@salimetrics.com • salimetrics.com